




SJ1-026US / A00E1220 Shankar et al. Implantable Cardiac Therapy Device with Dual Chamber Can to Isolate High-Frequency Circuitry

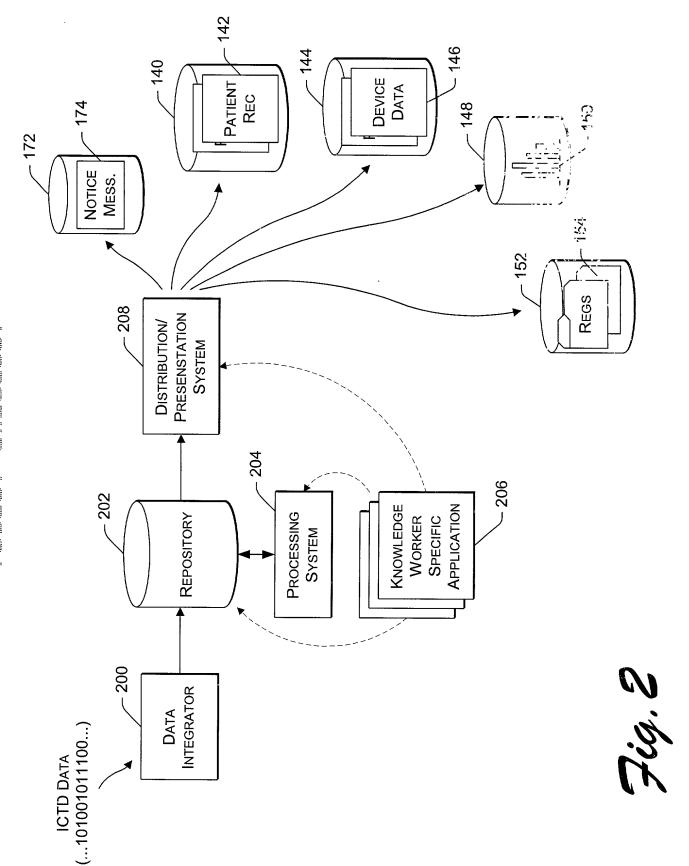

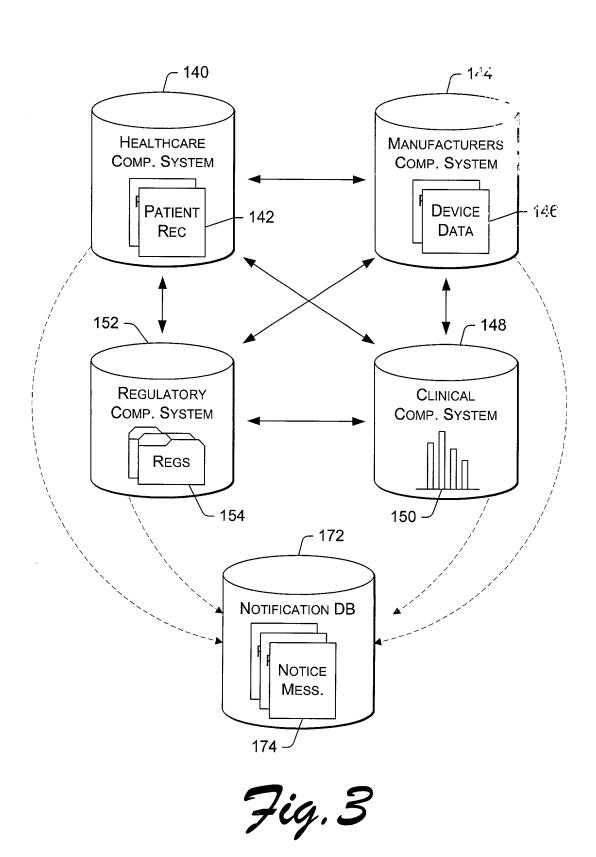

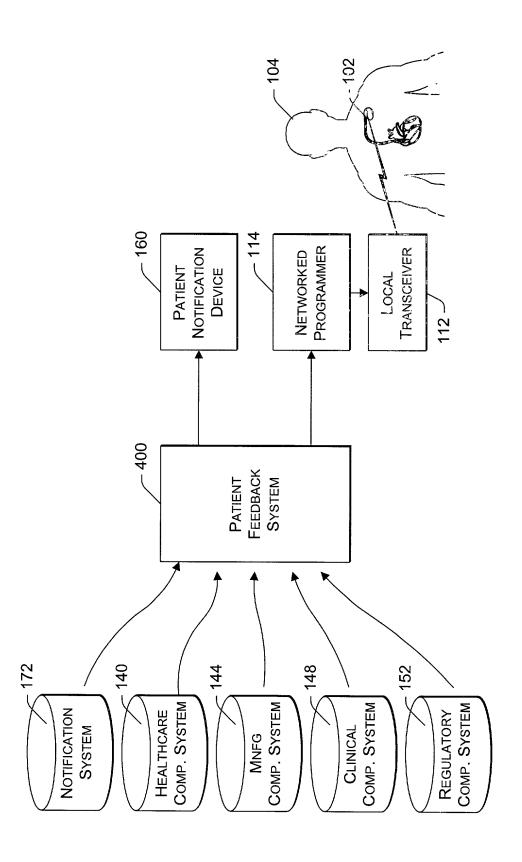

SJ1-026US / A00Ξ1220 Shankar et al. Implantable Cardiac Therapy Device with Dual Chamber Can to Isolate High-Frequency Circuitry

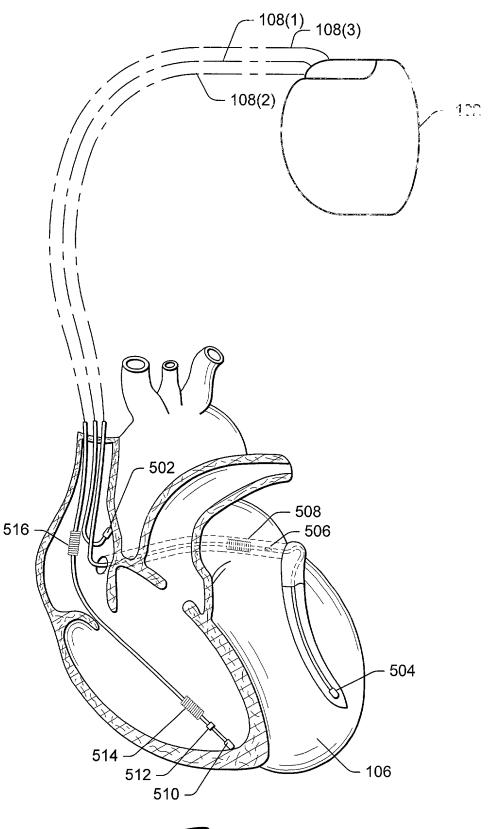
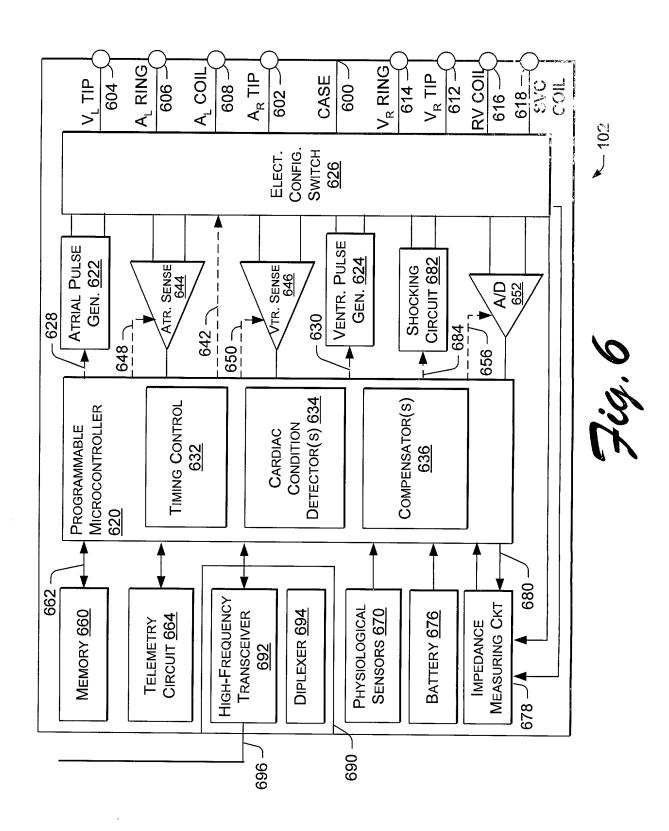


Fig.5



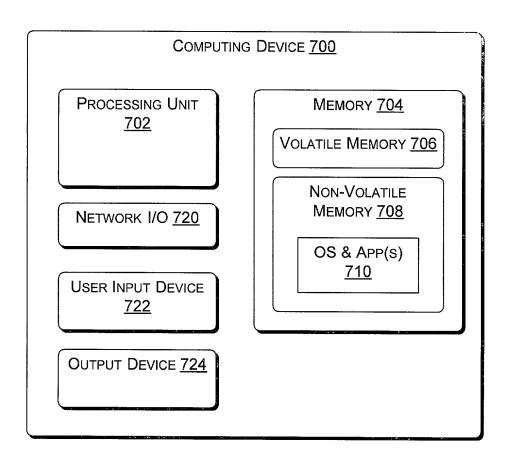


Fig. 7

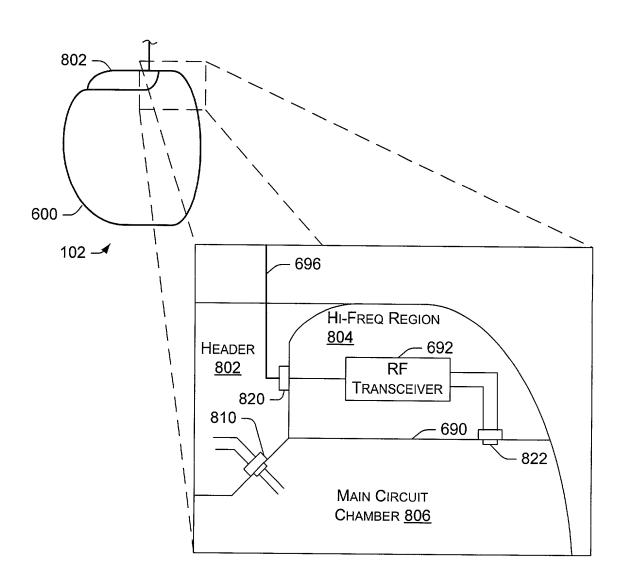


Fig. 8

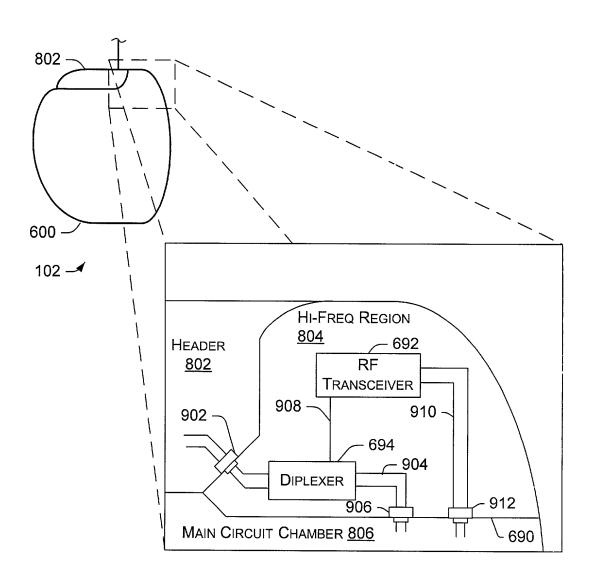
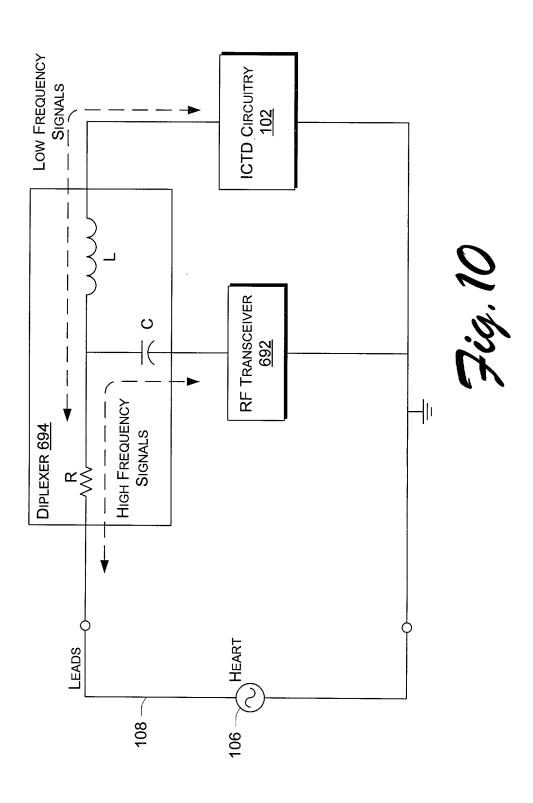
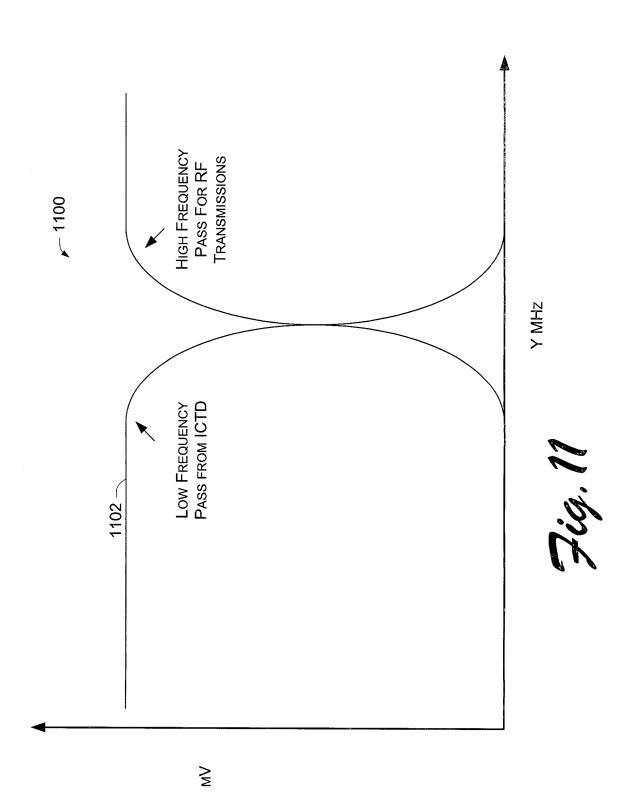


Fig. 9







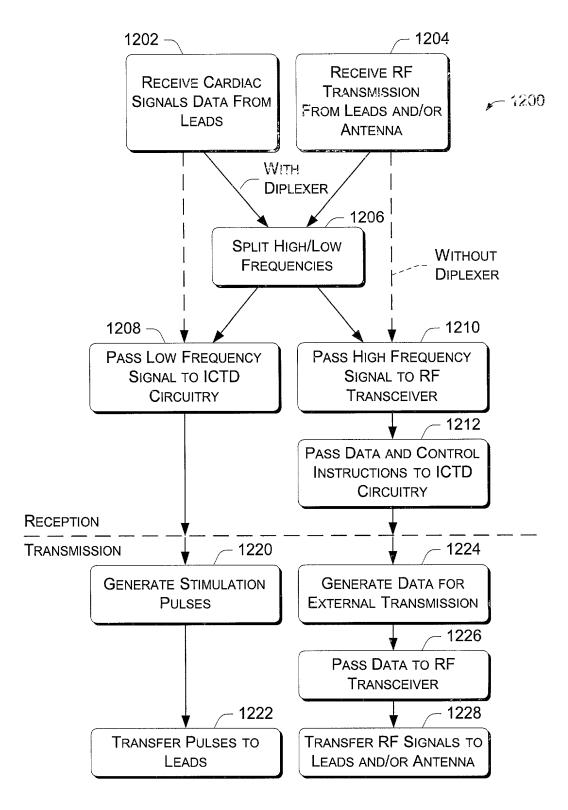


Fig.12